

Summit 11000/12000 B-Series Probe Station



Facility Planning Guide

This guide contains information to help prepare your facility for the arrival of your Cascade Microtech, Inc. probe station.


Probe Station Requirements

| | | |
|---------------------------------|--|--|
| Air and Vacuum | Vacuum | <ul style="list-style-type: none"> • 400mmHg (15 inch of mercury) minimum • Minimum vacuum required: 3.4 liters/minute (0.12 SCFM) |
| | Vacuum connection | <ul style="list-style-type: none"> • 8 mm (0.315 in.) O.D. polyurethane tubing • 2.4 m (8 feet) provided |
| | Compressed air for High Stability Tilt-back Bridge | <ul style="list-style-type: none"> • 0.55-0.86 Mpa (80 - 125 psi) input |
| MicroChamber Purge | Available Flow | <ul style="list-style-type: none"> • 170 liters/minute (6 SCFM) maximum; 113 liters/minute (4 SCFM) if using nitrogen for "quickpurge" • Continuous operation requires less air; 57-85 liters/minute (2-3 SCFM) |
| | Purge Connection | <ul style="list-style-type: none"> • 12.7 mm (0.50 inch) O.D. polyurethane tubing (PN 112-405) 3 meters (10 feet) is provided in the Accessories Kit |
| | Dew Point (Dry Air or Nitrogen) | <ul style="list-style-type: none"> • < -70°C |
| Environmental Conditions | Operating | <ul style="list-style-type: none"> • Altitude up to 2000 m • Main supply voltage fluctuations not to exceed $\pm 10\%$ of the nominal voltage • A total current of 3.2/1.6 A, 115/230 VAC is required for both auxiliary and microscope outlets. The combined leakage current of accessories attached to these two outlets must be less than 3mA. |
| | Temperature | <ul style="list-style-type: none"> • 20-30°C |
| | Humidity | <ul style="list-style-type: none"> • 0-95% noncondensing. |
| | Seismic restraints | Installation of seismic restraints is required to safely restrain the probe station during a seismic event and to meet the safety requirements as outlined by SEMI-S2. |
| Power | Outlets | <ul style="list-style-type: none"> • One (1) outlet is required for the IEC power cord kit/block: 115 V at 4 A (minimum), or 230 V at 2 A (minimum). |
| | Cable | <ul style="list-style-type: none"> • For international shipments, the probe station will be supplied with appropriate power cables. |
| | Power requirements for accessories | <ul style="list-style-type: none"> • Vacuum pump 1 A / 0.5 A • Air compressor 3 A / 1.5 A • Video camera 0.5 A / 0.25 A • Laser 6 A / 3 A • Laser illuminator 3 A / 1.5 A • Microscope illuminator 2.5 A / 1.25 A • Computer 1.5A / 0.75A typical • Computer monitor 1.5A / 0.75A typical |
| Additional Equipment | Workbench | <ul style="list-style-type: none"> • Size: 1.2 m (4 feet) wide x 0.76 m (2.5 feet) deep minimum • Capacity: 230 kg (507-pound) minimum |
| | Flowmeter | <ul style="list-style-type: none"> • Omega Model # FL 4513-V (or equivalent), 0-8 SCFM air flow (standard on Summit -AP and -M microchamber stations, optional and ordered separately for Summit -S stations) • The flowmeter is not required if an air dryer is included in the system configuration. • If a MicroChamber is included in the system configuration, a flowmeter is included for purge air control. Specifications for the flowmeter are 0 to 8 CFM. |

Summit 11000/12000 B-Series Probe Station


| | | |
|---------------------------------------|------------------------------|--|
| Dimensions | 11000 B-series probe station | <ul style="list-style-type: none"> • Approx. 81.5 cm/32.09 in. (W) x 76.2 cm/30 in. (D) • Station height: approx. 36.8 cm/14.5 in. (see height with microscopes on page 3) |
| | 12000 B-series probe station | <ul style="list-style-type: none"> • Approx. 82.5 cm/32.48 in. (W) x 76.2 cm/30 in. (D) • Station height: approx. 36.8 cm/14.5 in. (see height with microscopes on page 3) |
| Weight | Probe station | <ul style="list-style-type: none"> • 182 kg |
| | Lifting requirements | To avoid personal injury and/or damage to the station, a forklift (minimum 400-pound capacity) is required to move the unit, and a minimum of four to six people will be required to shift it onto the table. Note that the weight is not distributed evenly between all four corners of the station. The rear of the station is heavier than the front. |
| Shipping Dimensions and Weight | Station and table | <ul style="list-style-type: none"> • 90.2 cm/35.5 in. (W) x 106.7 cm/42 in. (D) x 90.4 cm/35.6 in. (H) |
| | Station and crate | <ul style="list-style-type: none"> • Weight: 272 kg (600 pounds) |

Front view

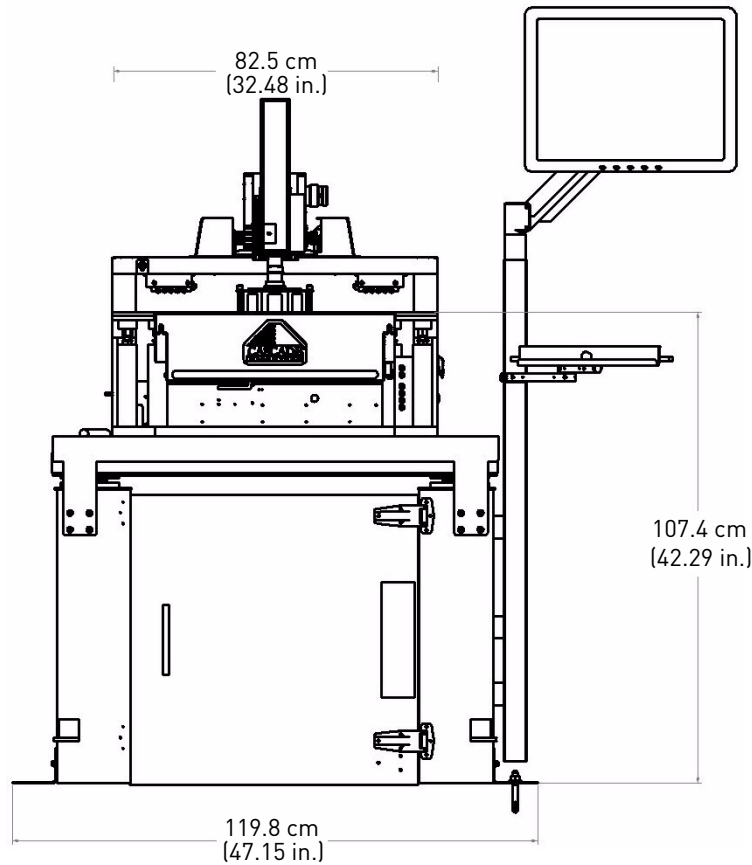


Summit 11000/12000 B-Series Probe Station

Side view with monitor on stand

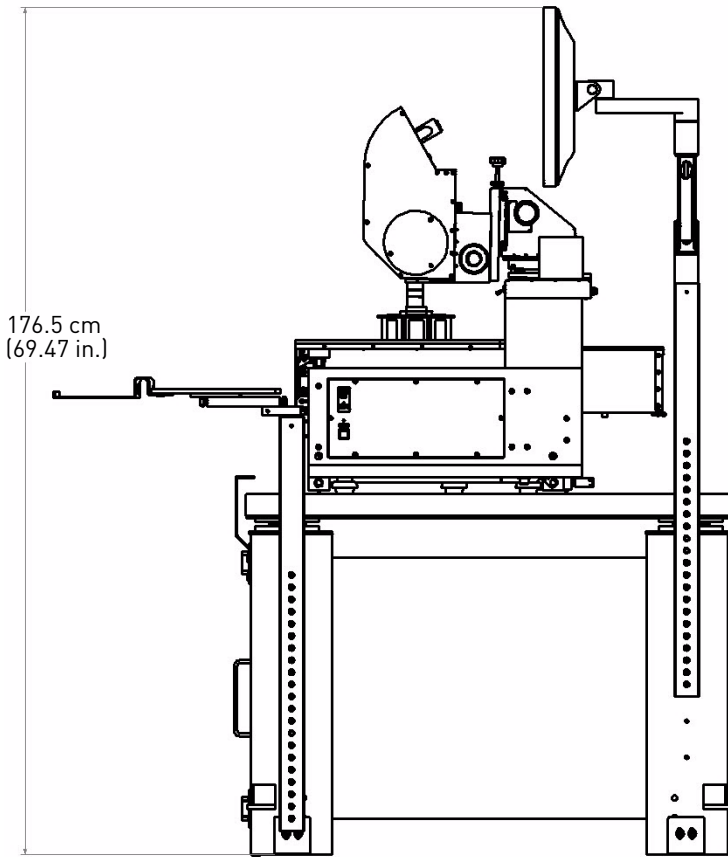

Side view with eVue in raised position

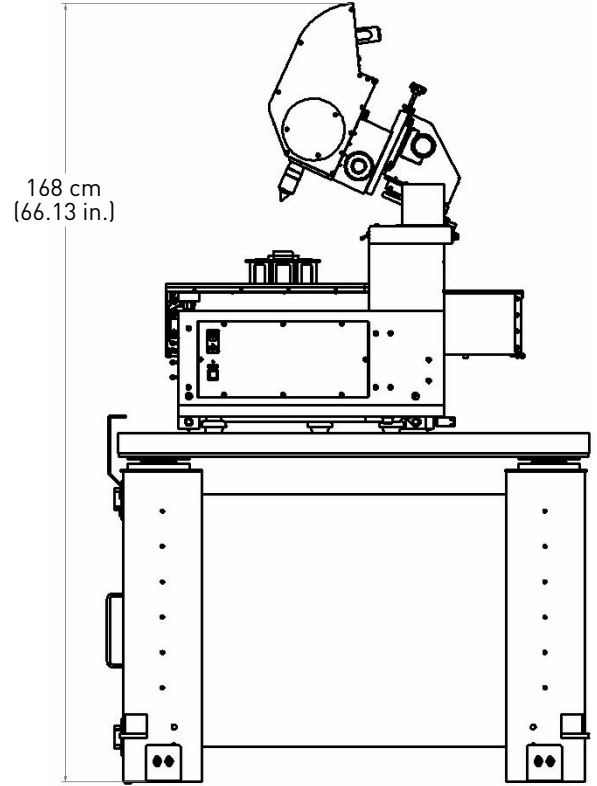

NOTE

| | |
|---|----------------------|
| Height with eVue in lowered position | 156.1 cm (61.44 in.) |
| Height with eVue in raised position | 168 cm (66.13 in.) |
| Height with monitor on monitor stand | 176.5 cm (69.47 in.) |
| Height with Mitutoyo microscope and installed laser | 184 cm (72.45 in.) |

© Copyright 2011 Cascade Microtech, Inc. All rights reserved. Cascade Microtech is a registered trademark of Cascade Microtech, Inc. All other trademarks are the property of their respective owners.

Data subject to change without notice.

Cascade Microtech, Inc.
Corporate Headquarters
 toll free: +1-800-550-3279
 phone: +1-503-601-1000
 email: cmi_sales@cmicro.com

Germany
 phone: +49-89-9090195-0
 email: cmg_sales@cmicro.com

Japan
 phone: +81-3-5615-5150
 email: cmj_sales@cmicro.com

China
 phone: +86-21-3330-3188
 email: cmc_sales@cmicro.com

Singapore
 phone: +65-6873-7482
 email: cms_sales@cmicro.com

Taiwan
 phone: +886-3-5722810
 email: cmt_sales@cmicro.com

